Chemical Hygiene Plan

Colgate University
Environmental Health and Safety
13 Oak Drive, Hamilton, NY 13346

Last Updated: January 2023

THIS PAGE INTENTIONALLY LEFT BLANK

Biological / Medical Waste
Radioactive Wastes
Used Laboratory Gloves
Empty Chemical Containers
Universal Waste Management
Accidents, Chemical Spills, and Emergency Procedures 31
Incidental Spill Procedures
Universal Emergency Response Procedures
Definitions 34

Appendices
Appendix A: Example Laboratory Hazard Assessment 36
Appendix B: ANSI 287.1 37
Appendix C: General Chemical Resistance Chart for Gloves 38
Appendix D: General Chemical Compatibility Guidelines 42
Appendix E: CHP Annual Review and Amendments 43

Introduction

The Occupational Safety and Health Administration (OSHA) regulation entitled "Occupational Exposure to Hazardous Chemicals in Laboratories" (29 CFR 1910.1450), commonly referred to as the Laboratory Standard, requires all employers engaged in the laboratory use of hazardous chemicals to develop and implement the provisions of a Chemical Hygiene Plan (CHP) that is capable of protecting workers from the health hazards associated with the hazardous chemicals used in that particular workplace.

This CHP applies to all laboratories and all laboratory workers at Colgate University. This includes, but is not limited to, teaching and research laboratories in the Departments of Art and Art History, Biology, Chemistry, Geology, Physics and Astronomy, and Psychology. OSHA defines a laboratory as "a workplace where relatively small quantities of hazardous chemicals are used on a non-production basis."

The effectiveness of Colgate University's CHP will be reviewed at least annually and updated as necessary.

- Follow all lab -specific operating procedures, including use of personal protective equipment

General Procedures for Working in a Laboratory

Personal Hygiene

- Do not prepare, store, or consume food or beverages in the laboratory
- Do not apply cosmetics in the laboratory
- Do not smoke in any laboratory or have tobacco produc ts in open packages
- Wash hands and lower arms before leaving the lab oratory , even if gloves were worn
- Do not pipette or siphon by mouth
- Sandals, open toed shoes, shorts, and skirts must not be worn in laboratories
- Appropriate personal protective equipment (PPE) shall be worn
- Hair past shoulder length shall be tied back and loose jewelry should be removed
- Do not wear or take glove s, lab coats , or lab aprons outside of the laboratory without faculty or staff approval

Housekeeping

- Work areas shall be kept clean and aisles must be free from obstructions
- Access to emergency equipment, exits, and control panels shall be kept clear at all times
- Universal precautions require that gloves are disposed of in the provided step cans
- All chemical containers (including waste containers) shall be properly labeled
- Spilled chemicals shall be cleaned up and disposed of properly
- Hazardous waste containers are removed from the laboratory by EHS

Experim ent in Progress

- Equipment such as hot plates, heating mantles, and water condensers shall not run unattended without fail -safe provisions
- Unattended operations and experiments shall be checked regularly
- Appropriate signage (avail fgress

- Adequate hand protection shall be worn when inserting glass tubing into rubber stoppers or corks, or when placing rubber tub ing on glass connections
- Glass apparatuses under vacuum shall be handled with extreme care to prevent implosion
- Glassware or bottles used in laboratory operations shall not be used for food or beverages
- Collect all used needles and syringes in designated r ed sharps containers

Systems under Pressure

- Reactions under pressure shall be carried out in an apparatus that is designed to withstand the full pressure of the system
- All pressurized apparatuses shall have appropriate relief devices

Compressed Gases

- Gas cylinders shall be strapped or chained securely to a wall or bench top
- Gas cylinders shal l be transported using cylinder carts designed specifically for this purpose
- An appropriate regulator shall be used and g as cylinders shall be capped when not in use
- Flammable compressed gases

non-inhibited material must be stored, then material should be stored under an inert atmosphere.

- Do not store peroxide forming materials in clear glass bottles (light can accelerate peroxide formation). It is recommended that an amber transparent bottle be used. Do not store the material in a metal can or other container that must be opened to see inside.
- Do not store peroxide -forming chemicals near heat , sunlight, or ignition sources. Avoid places that undergo temperature variations that can cause the bottle to “breathe in” oxygen.
- Do not distill, evaporate or concentrate the material unless it has been tested for the presence of peroxides. Peroxides ar e usually less volatile than their parent material and tend to concentrate upon distillation.
- Never touch or attempt to open a container of a peroxide -forming liquid if there are crystals around the cap and/or in the bottle. Place the container in safe st orage and contact EHS immediately.

Classes of Hazardous Chemicals

The hazard class of a chemical provides information to help determine how it can be safely stored and handled. Each chemical container m

- Oxidizers "may, generally by yielding oxygen, cause, or contribute to, the combustion of other materials."
- Pyrophoric materials, "even in small quantities, are liable to ignite within five minutes after coming into contact with air."
- Water-reactive materials are chemicals that "react with water to release a gas that is either flammable or presents a health hazard."

Health Hazards

OSHA defines a health hazard as a chemical for which there is significant evidence that acute or chronic health effects may occur in an exposed employee. TD[(on943 w 0.029 Tc 0.001 T

provide guidance on appropriate levels of PPE ac ross the range of experimental procedures encountered in the research setting.

Eye and Face Protection

Eye and face protection is to be worn by all persons whenever any one person in the laboratory is conducting an activity that involves potential eye and face hazards. Activities that present potential eye and face hazards include, but are not limited to , work involving the following:

- Hazardous chemicals
- Flying particles
- Hot solids, liquids, or molten metals
- Milling, sawing, turn ing, shaping, cutting, or stamping of any solid materials
- Heat treatment, tempering, or kiln firing of any metal or other materials
- Gas or electric welding
- P

Hand Protection

Gloves are to be used when handling hazardous chemicals in the laboratories. Typically, the requirements of the general laboratory hazard assessment should be followed. However, deviations may be made as outlined in the parag raph on experiment specific laboratory hazard assessments. EHS can provide guidance on appropriate hand protection i n instructional and research settings. There is no

Protective Clothing

Lab coats and lab aprons prevent skin contact exposure to chemicals by providing a protective barrier between the hazard and the laboratory user's torso, waist , and extremities.

Lab Coats

Lab coats are to be used when handling hazardous chemicals in the laboratories. Typically, the requirements of the general laboratory hazard assessment should be followed. However, deviations may be made as outlined in the paragraph on experiment spe cific laboratory hazard assessments. EHS can provide guidance on appropriate protective clothing in instructional and research lab settings. Faculty , staff, and student lab coats are provided and maintained by EHS . Colgate University's lab coats have the following protective qualities:

- Flame-resistant fabric
- High tensile strength thread material
- NFPA 70E, HRC 2 compliant
- Arc Rated to 8 cal /cm^2
- Thermal and electrical arc hazard rated to ASTM 1506 -02a standard
- Covered gripper snap front for quick and safe ga rment removal
- Covered gripper snap cuffs to prevent garment interference during chemical handling /experimentation work
- Lightweight (7 oz) lndura Ultra Soft fabric for unrestricted movement / user comfort
- 42 inches in length for maximum skin exposure prote ction

Lab coats are maintained, cleaned, and replaced, when necessary, by EHS . Lab coats wi ll be cleaned by a qualified commercial laundry service provider at the end of each semester and at the end of the summer to ensure periodic removal of any p otentia l chemical contamina nt s. Additional cleanings will be coordinated by EHS as necessary upon request. In the event a lab coat becomes contaminated, deteriorated, or dam aged prior to the scheduled tri -annual cleaning, contact EHS for replacement and/or dispos al of the garment.

Lab Apron

Plastic or rubber lab aprons provide additional protection from skin contact exposure to

contaminated with harmful dusts, fogs, fumes, mists, gases, smokes, sprays, [and] vapors" (29 CFR 1910.134(a)(l)).

Colgate University shall first seek to prevent atmospheric contamination by implementing engineering controls whenever possible, prior to utilizing personal protective equipment (PPE).

Engineering controls can include enclosing the work area, introdu cing ventilation (mechanical ⁄ natural and local ⁄ general), and substitution of less toxic materials. After engineering controls are in place, respiratory PPE can be employed if deemed necessary. If respirators must be used to make the work environment sa fe, then their use shall be governed by the written, worksite specific Respiratory P rotection Program (RPP). The RPP describes all aspects pertaining to the safe use and

Engineering Controls and Safety Equipment

Fume Hoods and Ventilation

General ventilation provides only modest protection against inhalation hazards, and therefore will not be used for protection against toxins. Chemical fume hoods must be used to prevent harmful fumes, mists, dusts, gases, and vapors from entering the laboratory air. Fume hoods will be inspected and validated annually by trained Colgate representatives. Fume hoods are equipped with face velocity and sash height monitors that initiate an audible alarm when exhaust flow is at an unsafe condition. Fume hoods will maintain a face velocity between 80-120 linear feet per minute , with a calibrated performance bias, between 6" and 18" sash heights.

If a hood is found to be deficient , a warning sign indicating that the hood did not pass inspection and does not provide adequate protection will be attached in a conspicuous location. Under no circumstances should laboratory personnel continue to use a fume hood that has not passed the annual inspection/certification process, even if the fume hood appears to have airflow. Laboratory personnel must make arrangements with other laboratories that have functioning fume hoods if their work requires the use of a fume hood.

Work Practices for Chemical Fume Hoods:

- If you suspect that your fume hood is not functioning properly, alert EHS
- Set up work at least 6 inches from the face of the hood to avoid turbulence at the sash edge
- Separate and elevate each instrument by using blocks or racks so that air can flow(ev)04 (f)1 (l)7 i3T.p.47 (p)acksion. U fum wiacksion.els

- Sources of open flames, particularly Bunsen burners, present a potential fire or explosion hazard; electrical components of the BSC, such as the fan motor, lights, and electrical outlets are not designed to operate in flammable atmosphere, where a spark could ignite a flash fire.
- For inoculating bacterial cultures, sterile disposable loops or pipette tips are preferred; alternatively micro -burners or electric “furnaces” may be used.
- If deemed absolutely necessary for the work to be perfor med, PIs may petition the IBC to use a pilotless burner or safety touch -plate microburner, as an alternative to a Bunsen burner.

In the end, for ensuring sterility, the BSC is only as effective as its user. Best practices include:

- Maintaining annual certification of the hood
- Operating cabinet blowers for at least 3 -5 minutes prior to opening the sash to allow the BSC to purge particulates
- Using alcohol to clean the work surface of the BSC and to sterilize any glass being used; the amount of alcohol stored in the BSC shou (ol)6 ()-4 (iCo)-0.9en o ourabe By (l)

know the location and proper use of this equipment. In addition, the path to this equipment must not be obstructed. Laboratory users shall contact EHS or Facilities if they notice a nonfunctioning emergency eyewash or safety shower .

If the eyes and/or face are contaminated, immediately flush the eyes in the eyewash station for at least 15 minutes. The eyelids should be held open and eyeballs should be rolled around to fully irrigate the eye. If the body is contaminated, remove clothes at and below the affected area, and remain in the safety shower for at least 15 minutes. Contact Campus Safety and seek medical attention.

EHS posts appropriate signage indicating the presence of an eyewash and/or safety shower at each emergency station and performs periodic flushing of all eyewash stations. During a flush test, EHS visually inspc

indicates the extinguisher cannot be used on that class of fire. A missing symbol indicates the extinguisher has not been tested for that class of fire. Use of the wrong type of extingui sher can make the fire worse and endanger others .

Fire Extinguisher Operations:

- To operate a fire extinguisher, remember the word P.A.S.S.:
  - Pull the pin. Hold the extinguisher with the nozzle pointing away from you, and release the locking mechanism
  - Aim low. Point the exting uisher at the base of the fire

Training

Colgate University employees who work with hazardous chemicals, biologicals , and/or radiological materials require initial and periodic training appropriate to their level of responsibility. Faculty and staff must receive lab oratory safety training prior to working with hazardous chemicals, biologicals , and/or radiological materials , and on an annual basis. In addition, ge neral hazard communication information is presented to new employees who attend periodic new hire orientation sessions.

All students enrolled in a laboratory course or working in a laboratory setting are required to attend a Lab oratory Safety and Hazardou s Waste Management training session on a n annual basis. These training sessions are conducted by EHS at the beginning of each semester, and before summer research . Training covers the contents of the CHP and is divided into four sections: General Lab oratory Safety, Hazard Communication, Emergency Procedures, and Hazardous Waste Management. Students must sign a Laboratory Safety Agreement at the training session.

Special training is also provided by EHS upon request. Hazard -specific training is required if faculty, staff,

placed inside. Full containers shall be dropped off in the biological waste room, which is located in the McGregory Hall loading dock Bunker #3 . Upon drop off, the necessary information must be recorded on the Biological Waste Log. New sharps containers can also be picked up at that location.

thnebv . . M C /

Radioactive Wastes

- Rechargeable batteries such as nickel

Accidents , Chemical Spills , and Emergency Procedures

The HAZMAT Contingency Plan provides a written plan of action in the event of a fire, explosion, or unplanned release of hazardous materials or hazardous waste which could pose a threat to human health and/or the environment. Other documents, including Colgate University's Spill Prevention Control and Countermeasures (SPCC) Plan and Emergency Response Plan (ERP), may be used as additional resources during an incident involving hazardous materials or hazardous waste.

An incidental spill is defined by OSHA as a spill in which the substance can be absorbed, neutralized, or otherwise controlled at the time of release by employees in the immediate release area, or by maintenance personnel where there is no potential safety or health haz ard (i.e. fire, explosion, or chemical exposure). It is a release of a hazardous substance which does not pose a significant safety or health hazard to employees in the immediate vicinity or to the worker cleaning it up, nor does it have the potential to become an emergency within a short time frame. An incide ntal spill may be safely cleaned up by employees who are familiar with the hazards of the chemicals with which they are working.

the spill debris is located, and a

- Whenever a spill, leak, or other incident results in the likelihood of a hazardous exposure to a n employee or other laboratory worker.

All employees who work with hazardous chemicals must be given the opportunity to receive medical attention, including any follow-up examinations that the examining licensed physician decides are necessary. Employees will receive any medical examinations and consultations without cost or loss of pay and at a reasonable time and place. Certain information must be provided to the physician, including the identity of the hazardous chemicals, a description of the conditions under which the exposure occurred, and a description of the signs and symptoms of exposure that the employee is experiencing.

Appendix A: Example Laboratory Hazard Assessment

Appendix B: ANSI Z87.1



3

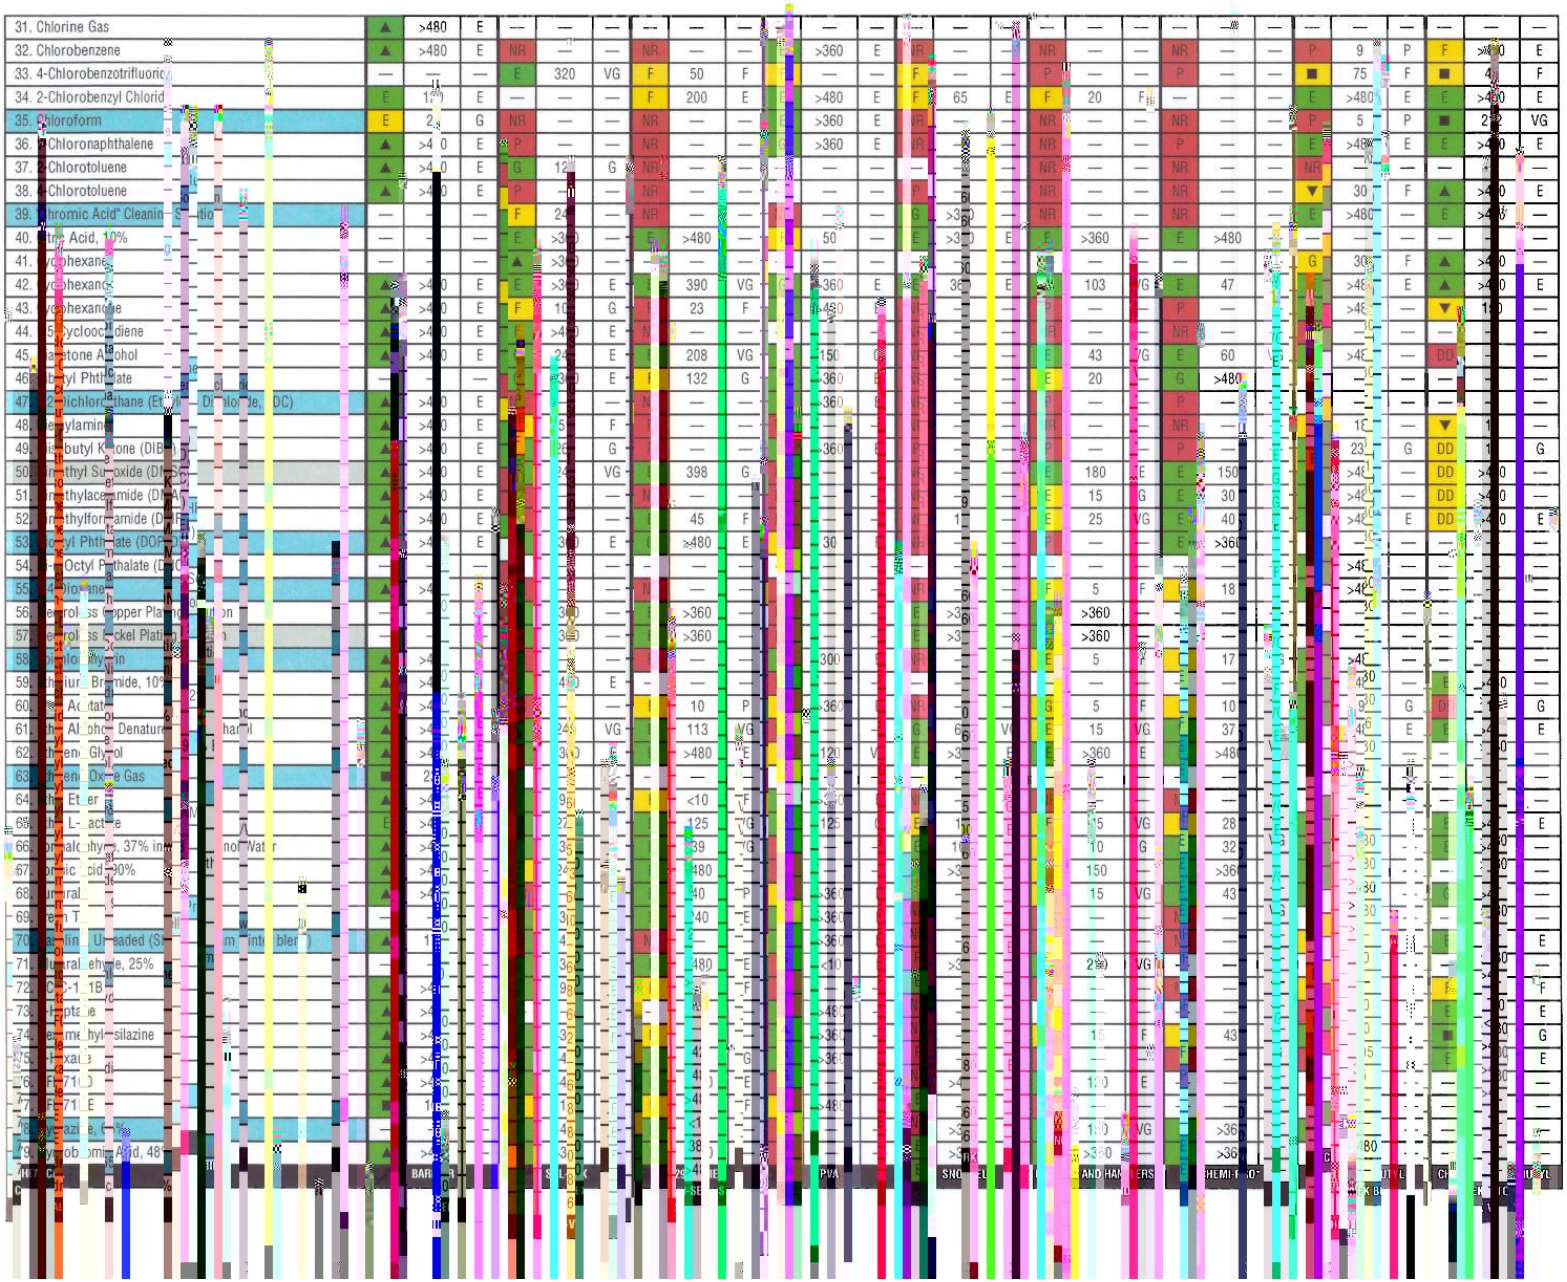

Appendix D: General Chemical Compatibility Guidelines

The following information is to be used only as a guide. Specific incompatibilities will be listed on the Material Safety Data Sheets.

Separate acids from

- Bases (possible violent exothermic reaction)
- Most metals (production of flammable hydrogen gas)
- Cyanides (forms toxic and fla mmable hydrogen cyanide gas)
- Sulfides (forms toxic and flammable hydrogen sulfide gas)
- Azides (may form explosive hydrazoic acid)
- Phosphides (may form toxic and flammable phosphene gas)
- Oxidizers (may form toxic and/or explosive compounds)

Separate oxidizers from

- Acids (may form toxic and/or explosive compounds) (For example: concentrated sulfuric acid mixed with chlorates or perchlorates forms explosive compounds)
- Organic materials (especially when mixed with flammables, may ignite)
- Metals (may form explosive compounds)
- Reducing agents (for example: boranes, hydrides, sodium hydrosulfite, etc.)
- Ammonia (anhydrous or aqueous)

Separate water -reactive chemicals from

- Aqueous solutions and in many cases just the moisture in the air (for example: metal hydrides, alkali metals and certain metal dusts in moist air will form hydrogen gas and ignite; halosilanes and acid halides will react with water to form toxic acid gases)

Separate Sodium Hypochlorite (bleach) from

- Acids (release of chlorine gas may occur)
- Solution containing ammonia (release of chlorine gas may occur, risk of explosive compounds)
- Organics (release of chlorine gas may occur, risk of explosive compounds)
- Metals (Pressurization may occur)
- Hydrogen Peroxide (violent release of oxygen gas may occur)
- Reducing Agents (heat reaction may occur)

Appendix E: CHP Annual Review and Amendments

Name: _____

Signature:___ _____

Title: _____

Review Date: _____

Updated? ‘ Yes ‘ No

If yes, provide a brief description of amendments and/or changes: _____

_____

_____

_____

Name: _____

Signature:___ _____

Title: _____

Review Date: _____

Updated? ‘ Yes ‘ No

If yes, provide a brief description of amendments and/or changes: _____

_____

_____

_____